

# TEST REPORT

Material Code: CT820a Chamber

Instrument IP: 192.168.1.21

Production: 2018

Test Date: 2/5/2018


Test Result: PASS

Instrument: Agilent Technologies, E5071C, MY46525444,B.13.10

## Data sheet:

| Frequency(GHZ) | Front   | Back    |
|----------------|---------|---------|
| 2.4GHZ         | -95.556 | -88.280 |
| 5.8GHZ         | -97.655 | -87.346 |

FRONT:

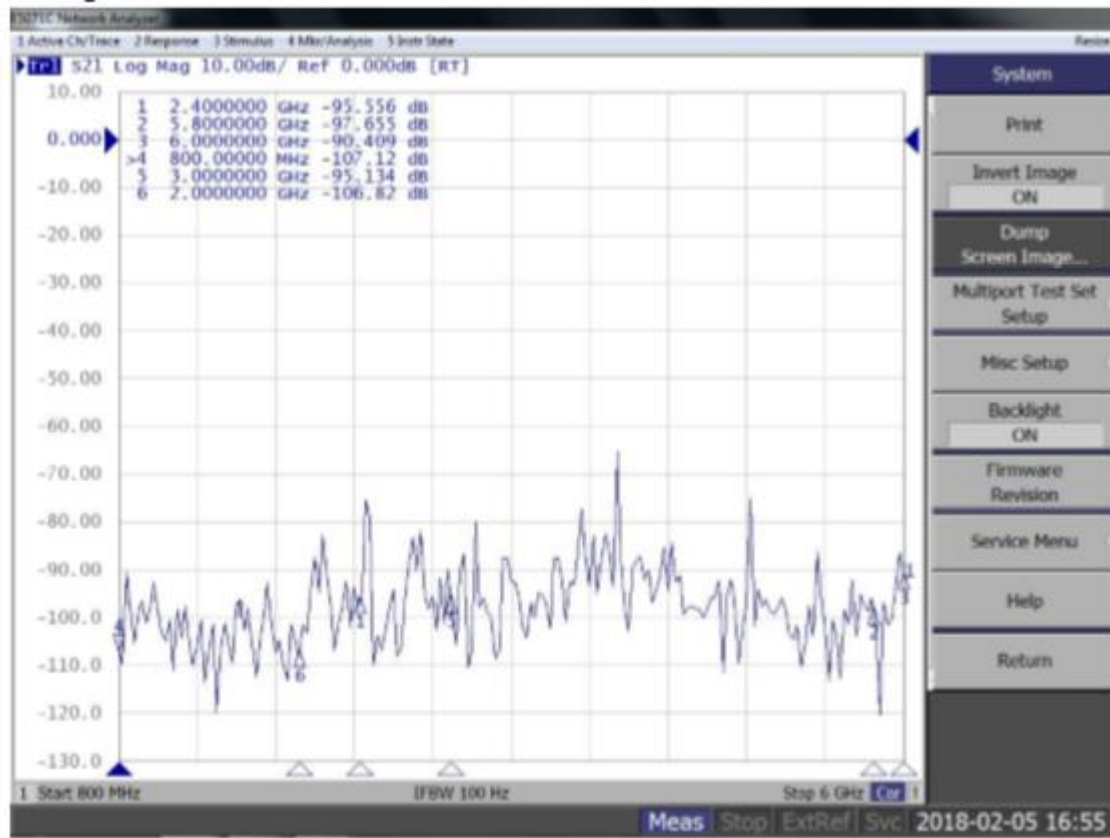

BACK:

